

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

SEP 21 2009

Supervisor/Operator Performing the Verification Procedure:	
Name	NICHOLAS YLINIEMI
ID#	3429
Date	9/16/09
Agency	METLAKATLA POLICE DEPT.
Phone #	886-4011
Instrument Location	METLAKATLA POLICE DEPT.
Alco S/N	X172942
Target Value	.084
High Pressure	900 ps'
Alco Test Values	.085
1 st Alco	.085
2 nd Alco	
Signature	Nicholas Yliniemi
(OVER)	

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Scientific Director
State Breath Alcohol Program


Subscribed and sworn before me this 16 day of Oct, 2009.

Carolyn M. Noland

Notary Public, State of Alaska

Commission Expires with Office

BT9 03/00

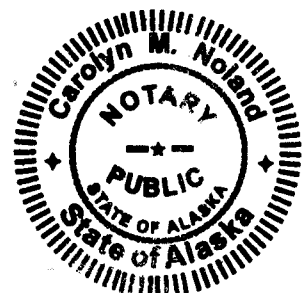

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130124

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130124

SEPTEMBER 16, 2009

OPERATOR'S NAME:

OLIVIERI, NICHOLAS/L

OPERATOR'S NUMBER: 3429

SUBJECT'S LAST NAME:

VER

SUBJECT'S FIRST NAME/MI :

OF CAL

O.L. #: 00000

DEPT/AGENCY MET:

TEST/REPORT: 00000

TEST TYPE: U

ALCO TARGET VALUE: .084

ALCO S/N: 2172342

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 20.54 IN

ALCO TARGET .084 09:59

BLANK TEST .000 09:59

INTERNAL STANDARD VERIFIED 09:59

ALCO TO 29.94 IN .065 10:00

BLANK TEST .000 10:01

SUBJECT SAMPLE .000 10:01

BLANK TEST .000 10:02

ALCO TO 29.94 IN .065 10:02

BLANK TEST .000 10:03

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130124

SEPTEMBER 16, 2009

TIME 09:57

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

WEIGHTS

SAMPLE NUMBER: 49c

TEST TUBE: 41c

BAROMETER: 29.94 in

ALCO DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

11/11/09 10:03:11 AM 130124 09:57 09:59 09:59 10:00 10:01 10:01 10:02 10:02 10:03
ALCO TARGET .084 ADJUSTED FOR 20.54 IN
BLANK TEST .000 09:59
INTERNAL STANDARD VERIFIED 09:59
ALCO TO 29.94 IN .065 10:00
BLANK TEST .000 10:01
SUBJECT SAMPLE .000 10:01
BLANK TEST .000 10:02
ALCO TO 29.94 IN .065 10:02
BLANK TEST .000 10:03